

High-frequency Heating Extraction Method for Sensitive Drug Analysis in Human nails

Fumiki Takahashi ^{1,*}, Masaru Kobayashi ², Atsushi Kobayashi ², Kanya Kobayashi ^{3,*} and Hideki Asamura ³

¹ Department of Chemistry, Faculty of Science, Shinshu University, 3-1-1 Asahi, Nagano 390-8621, Japan

² Research Institute of Scientific Criminal Investigation, Nagano Prefectural Police Headquarters, 3916 Nishijo, Matsushiro, Nagano 381-1232, Japan; takahashi@shinshu-u.ac.jp

³ Department of Legal Medicine, Shinshu University School of Medicine, 3-1-1 Asahi, Matsumoto, Nagano 390-8621, Japan; kanya_k@shinshu-u.ac.jp

* Correspondence: takahashi@shinshu-u.ac.jp (F.T.); Tel.: +81-263-37-2474

kanya_k@shinshu-u.ac.jp (K.K.); Tel.: +81-263-37-2474

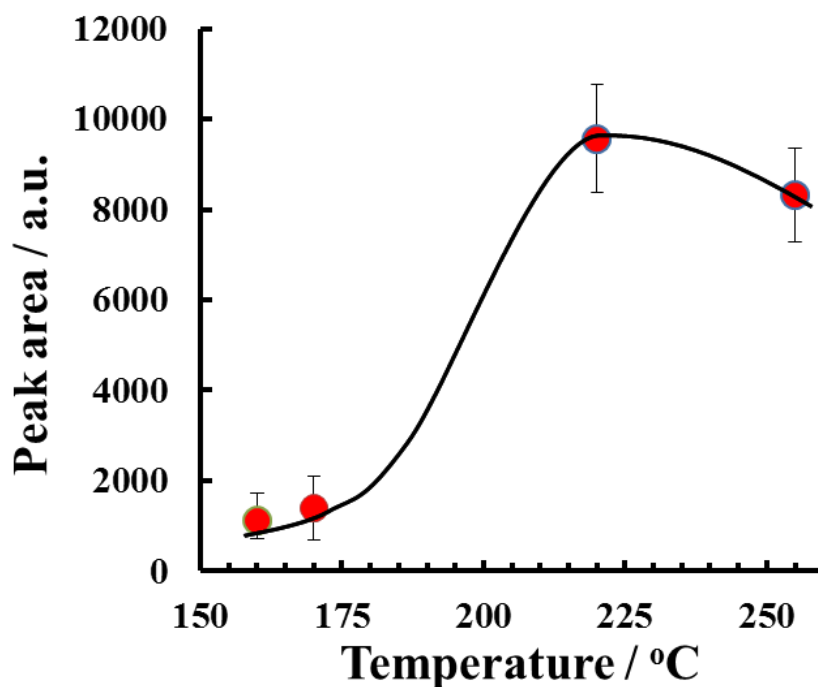


Figure S1. Dependence of the caffeine peak area on the extraction temperature for extraction of caffeine from nails. The sample mass was 10 mg and the H-F heating extraction was carried out at 220 °C. Error bars represent the standard deviation ($n = 3$).

Figure S1. F. Takahashi