

Supplementary Figure

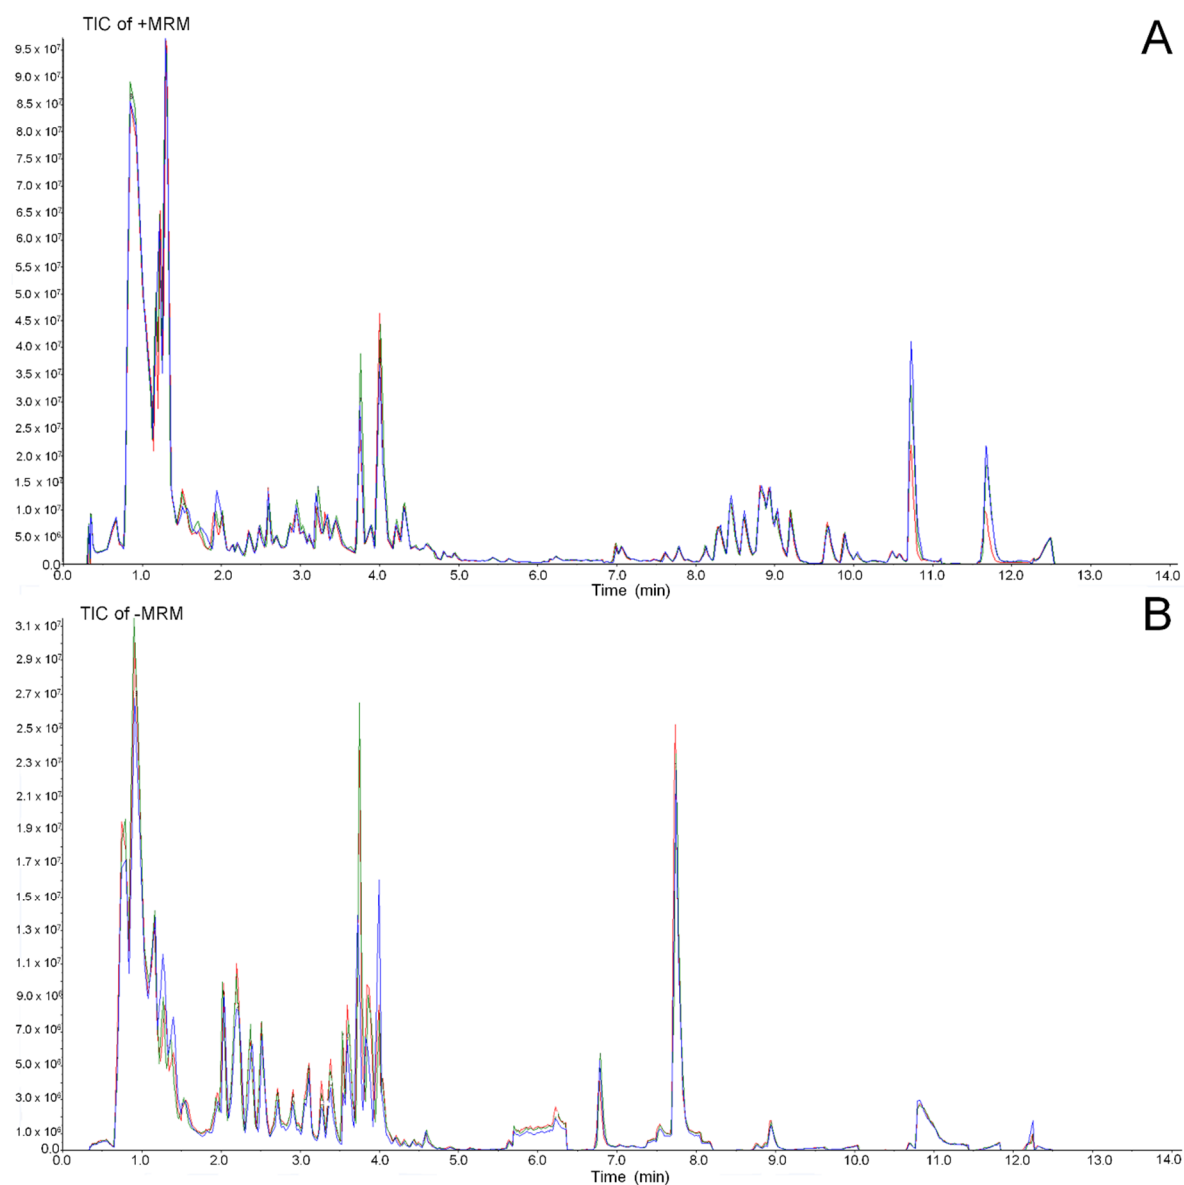


Figure S1. overlapping analysis of the TIC in QC samples. The x-axis represents the retention time (min) of metabolite detection, and the y-axis represents the intensity of ion current (cps: count per second). (A) for ESI⁺ mode; (B) for ESI⁻ mode.