


Supplementary Materials

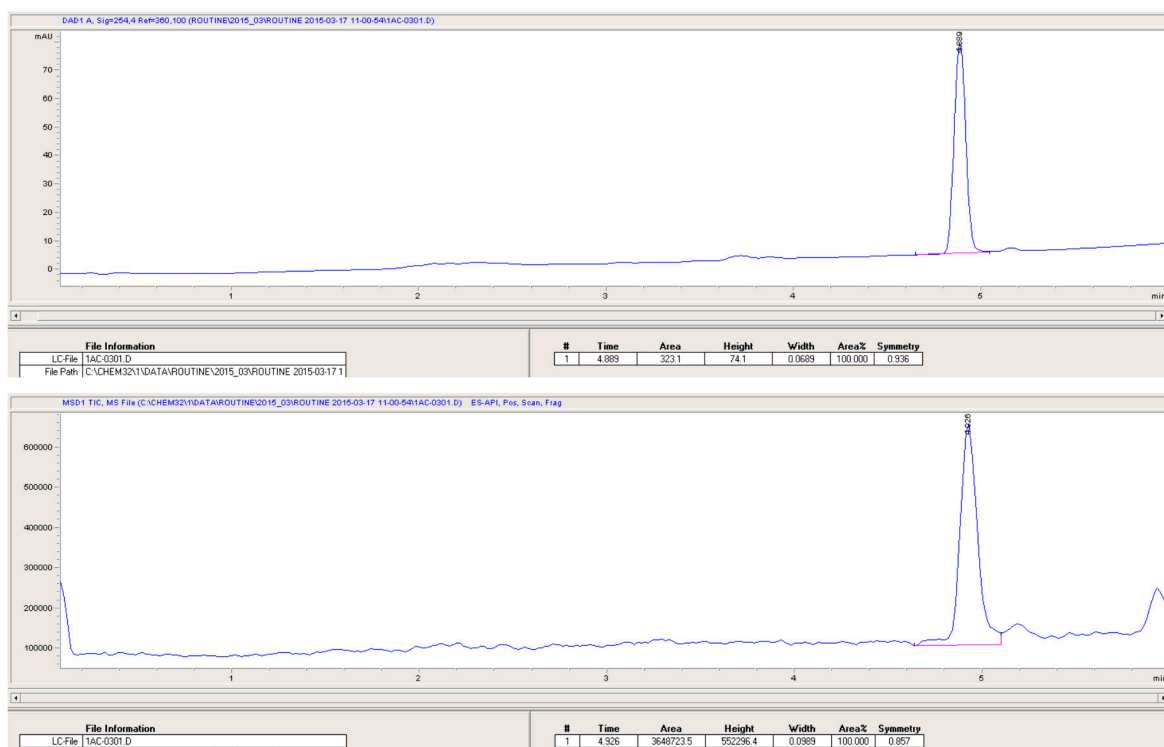

The purity of the final compound (greater than 95%) was determined by HPLC/MS on an Agilent 1290 system using a Agilent 1290 Infinity ZORBAX Eclipse Plus C18 column (2.1 mm × 50 mm, 1.8 μm particle size) with a gradient mobile phase of H₂O/CH₃CN (90:10, v/v) with 0.1% of formic acid to H₂O/CH₃CN (10:90, v/v) with 0.1% of formic acid at a flow rate of 0.5 mL/min, with UV monitoring at the wavelength of 254 nm with a run time of 10 min.

Figure S1. HPLC chromatograms.

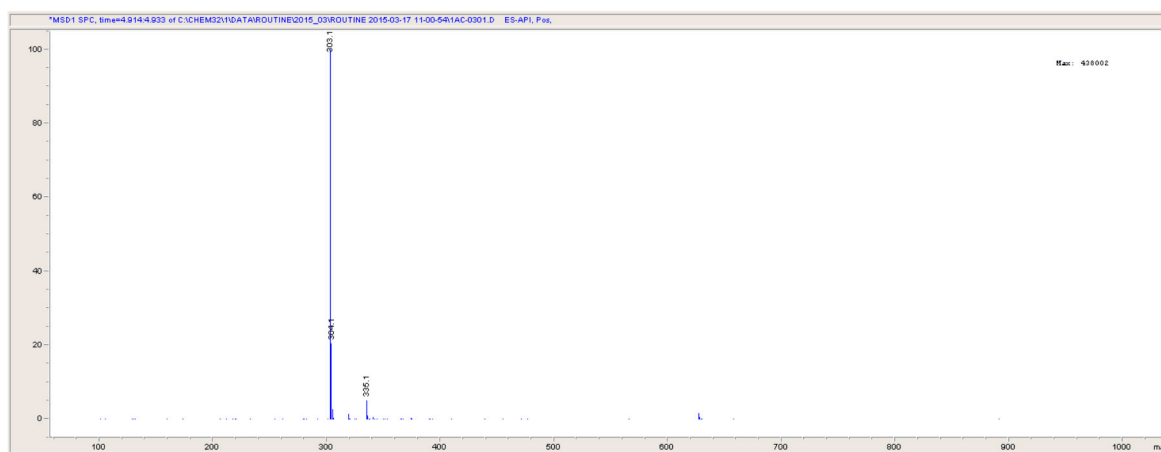
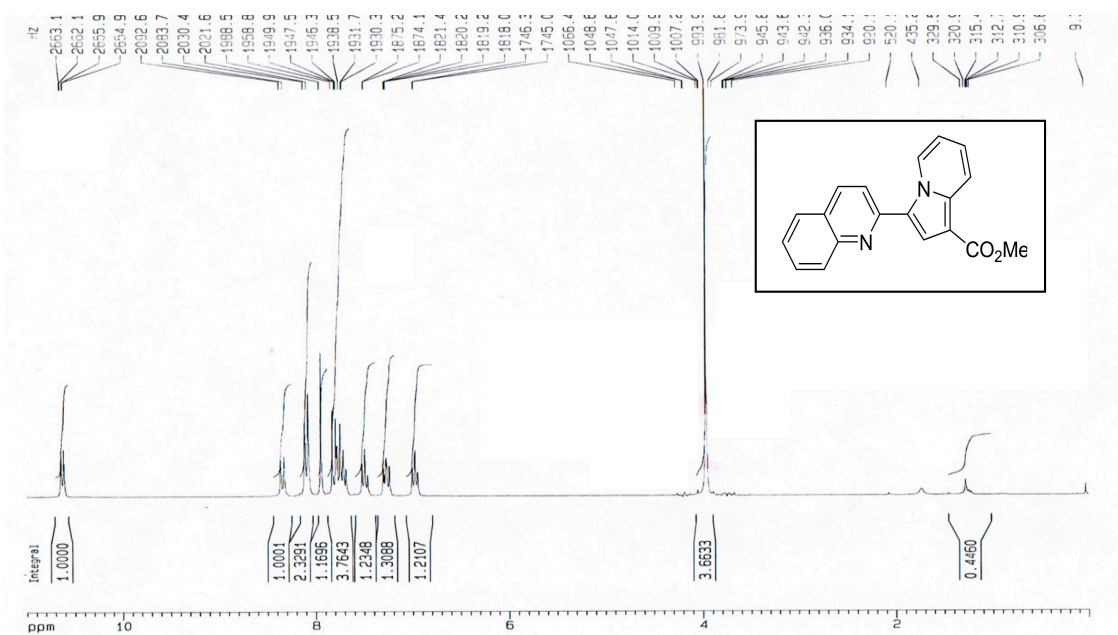
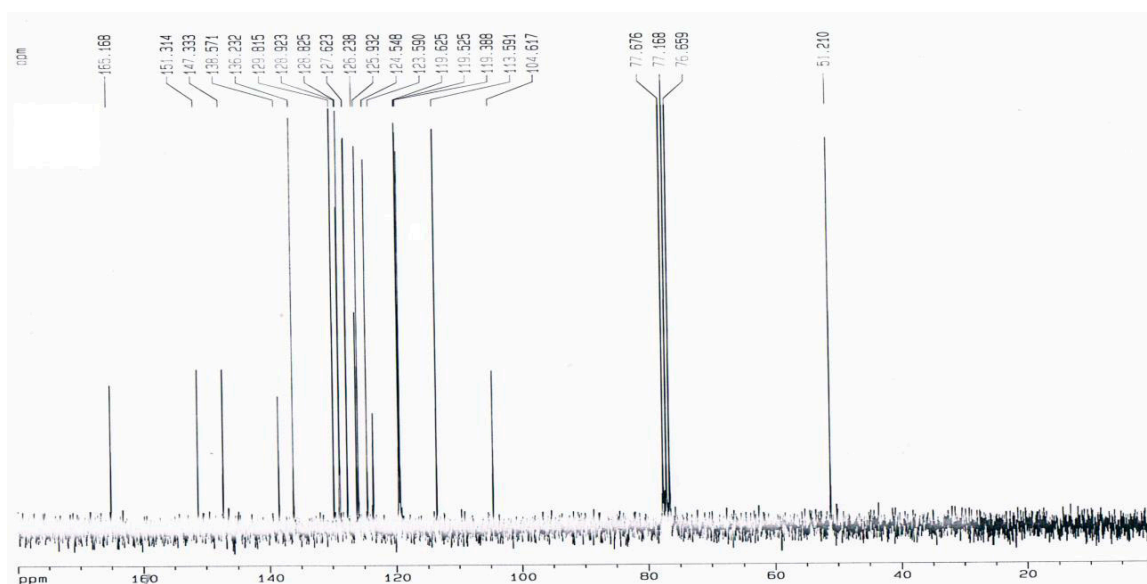


Figure S2. Mass spectra of compound 2.

Figure S3. ¹H-NMR spectra of compound 2.Figure S4. ¹³C-NMR spectra of compound 2.