


AK1101 sulfide

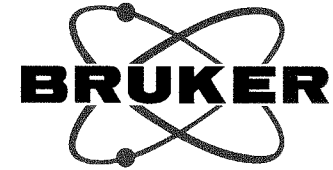


Current Data Parameters
 NAME Andreas Kalogirou
 EXPNO 557
 PROCNO 1


F2 - Acquisition Parameters
 Date_ 20140109
 Time_ 1.38
 INSTRUM spect
 PROBHD 5 mm PABBO BB-
 PULPROG jmod
 TD 65536
 SOLVENT CDC13
 NS 7000
 DS 4
 SWH 29761.904 Hz
 FIDRES 0.454131 Hz
 AQ 1.1010048 sec
 RG 2050
 DW 16.800 usec
 DE 6.50 usec
 TE 298.2 K
 CNST2 145.0000000
 CNST11 1.0000000
 D1 2.0000000 sec
 D20 0.00689655 sec
 TD0 1

==== CHANNEL f1 =====
 SFO1 125.7459782 MHz
 NUC1 13C
 P1 8.70 usec
 P2 17.40 usec
 PLW1 138.0000000 W

==== CHANNEL f2 =====
 SFO2 500.0350280 MHz
 NUC2 1H
 CPDPRG[2] waltz16
 PCPD2 80.00 usec
 PLW2 15.41699982 W
 PLW12 0.33258000 W

F2 - Processing parameters
 SI 32768
 SF 125.7334125 MHz
 WDW EM
 SSB 0
 LB 1.00 Hz
 GB 0
 PC 1.40

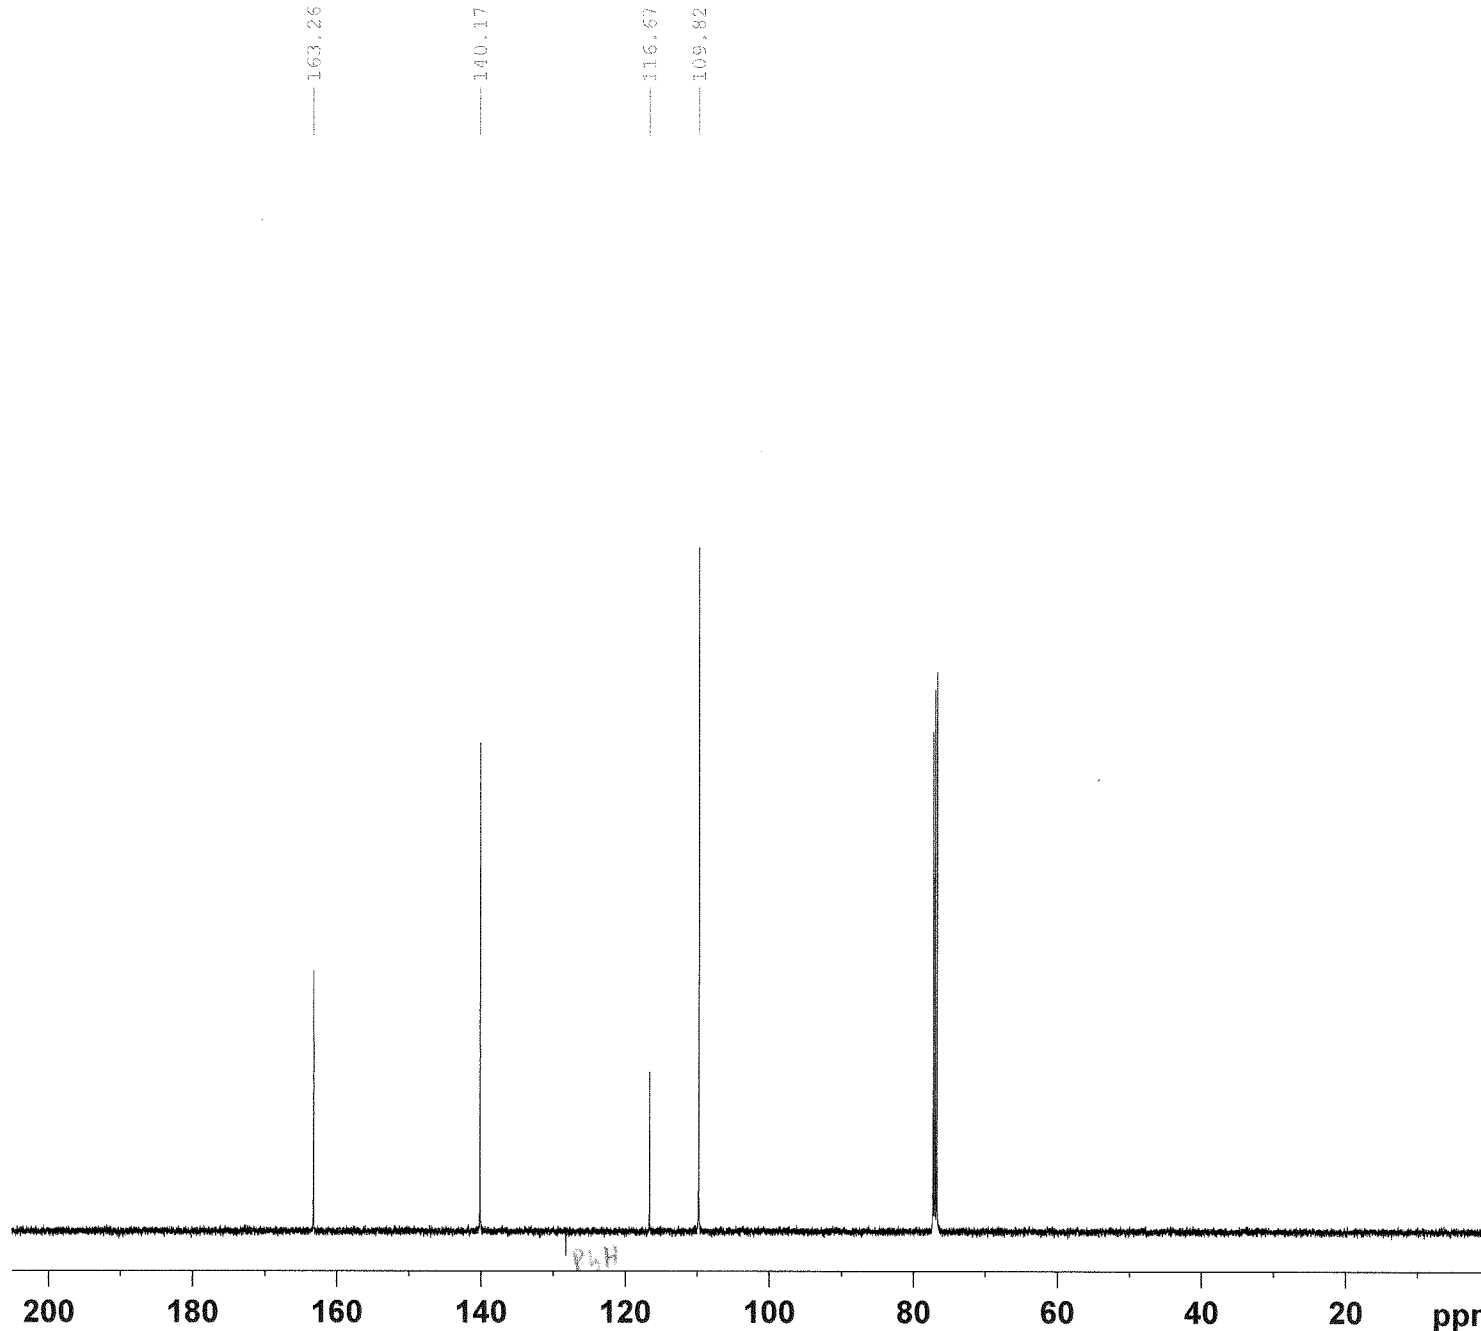

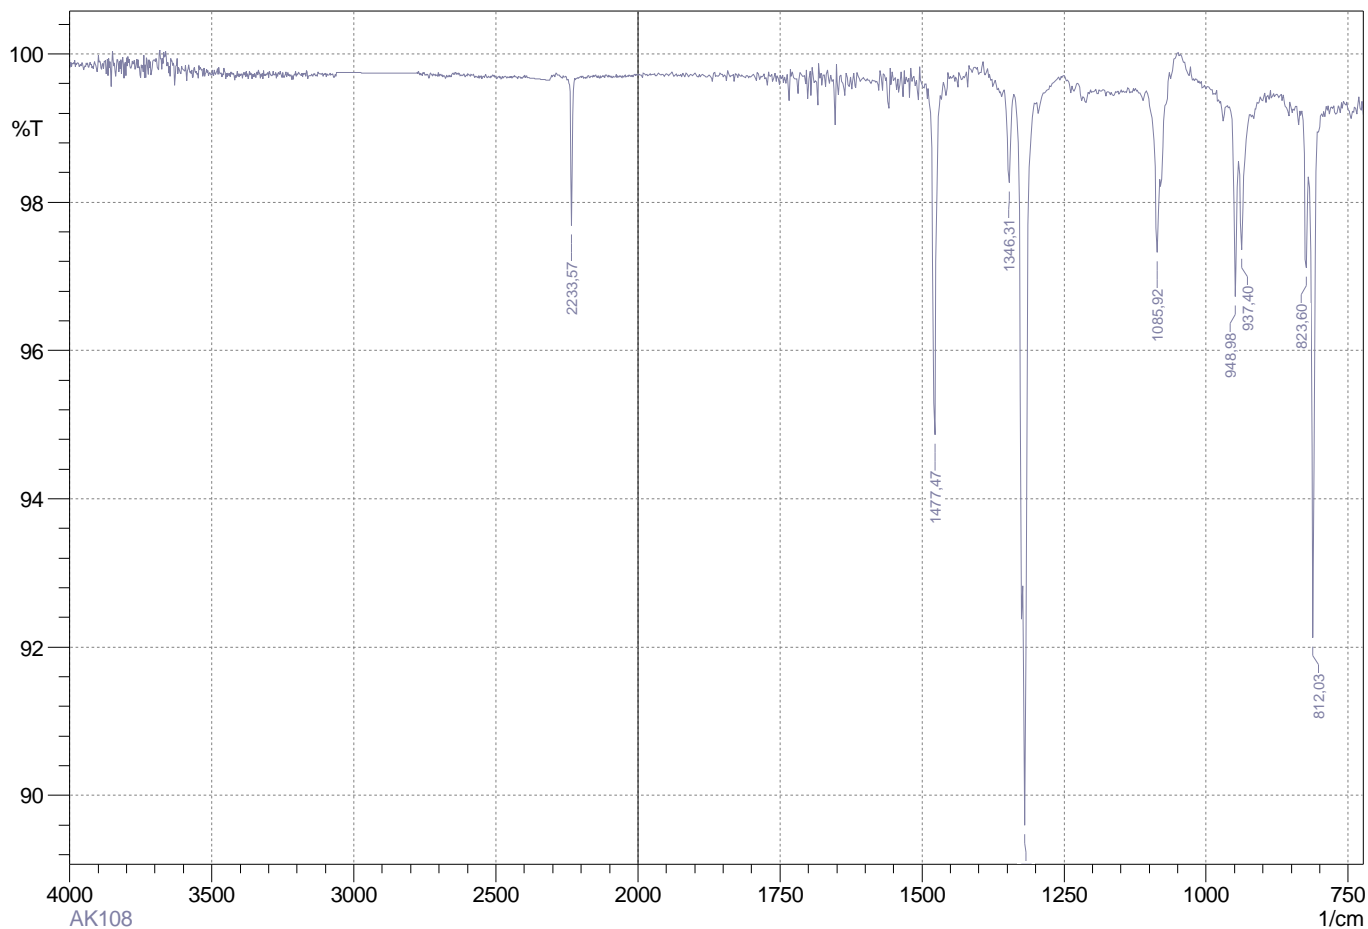

	Peak	Intensity	Corr. Intensity	Base (H)	Base (L)	Area	Corr. Area
1	812,03	92,129	6,391	817,82	804,32	0,23	0,149
2	823,6	97,116	1,523	831,32	819,75	0,093	0,032
3	937,4	97,358	1,363	943,19	921,97	0,142	0,036
4	948,98	96,726	2,1	958,62	943,19	0,118	0,045
5	1085,92	97,326	1,181	1105,21	1082,07	0,13	0,019
6	1319,31	89,593	3,033	1321,24	1301,95	0,271	0,04
7	1346,31	98,26	1,218	1355,96	1338,6	0,074	0,035
8	1477,47	94,86	4,715	1492,9	1463,97	0,206	0,153
9	2233,57	97,685	1,979	2247,07	2222	0,089	0,052