

Supplementary Materials

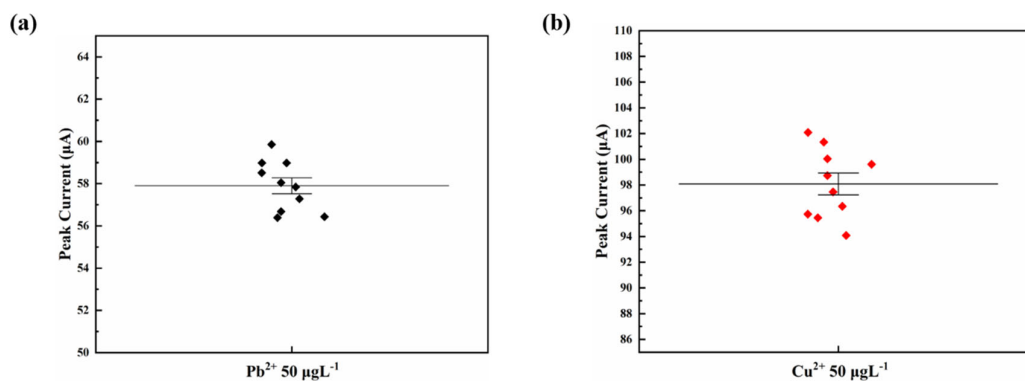


Figure S1. The detection results of 10 repeated tests for the individual determination of Pb^{2+} (a) and Cu^{2+} (b) with a concentration of $50 \mu\text{g/L}$.

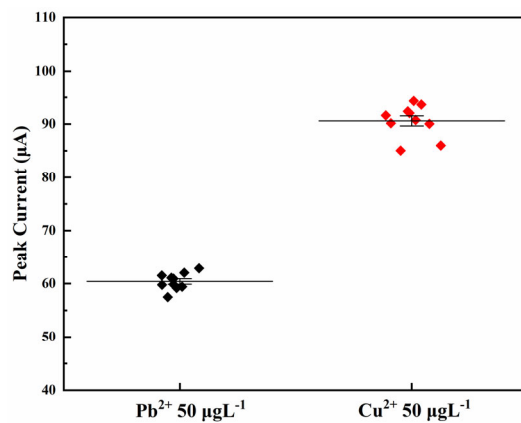


Figure S2. The detection results of 10 repeated tests for the simultaneous determination of Pb^{2+} and Cu^{2+} with a concentration of $50 \mu\text{g/L}$ each.