

Supplementary material



Figure S1. An example of a filter for measurements.



Figure S2. Measuring equipment PX-375 Horiba with other automatic analysers.

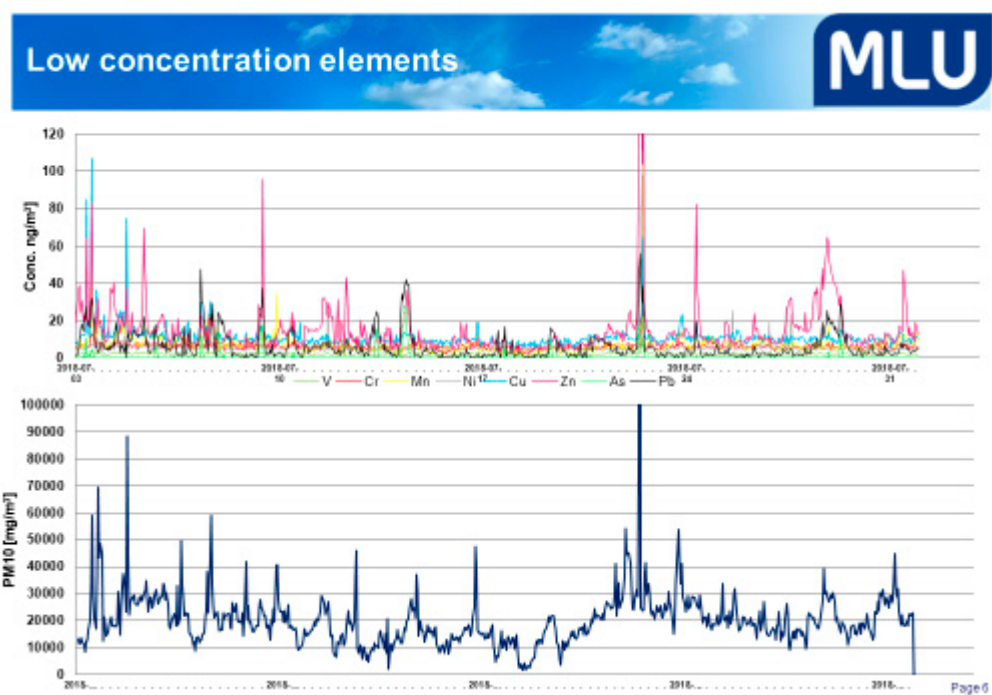


Figure S3. Measuring equipment PX-375 Horiba.

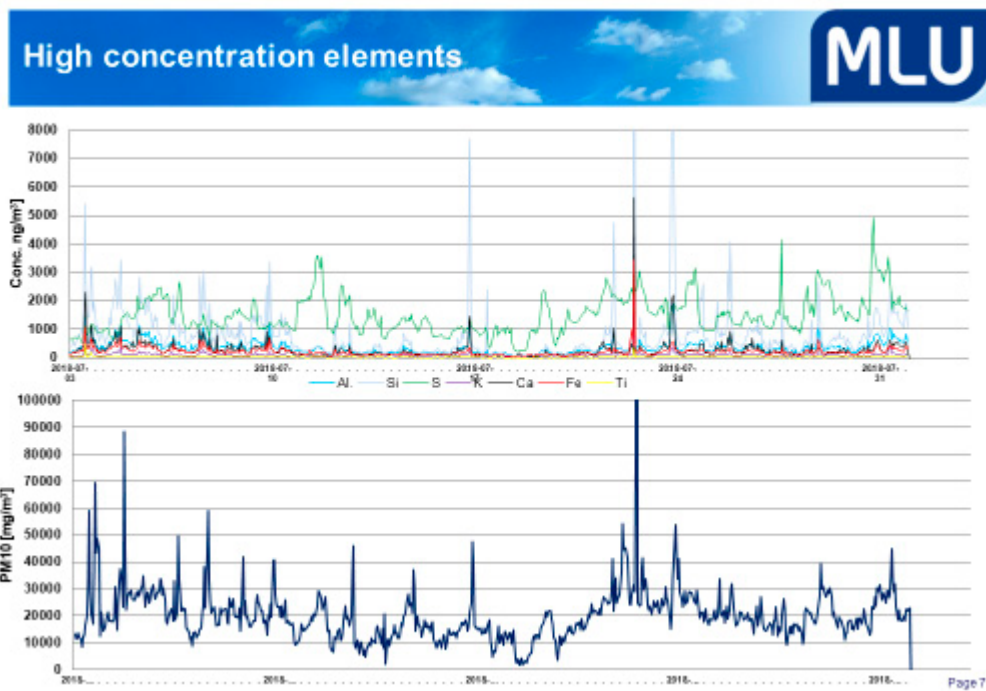




Figure S4. Sampling site in Kotórz Mały.



a.



b.

Figure S5a-b. The examples of obtained results. The concentrations of individual elements and PM10.