

Supplementary Materials

Microfluidic Droplet-Storage Array

Hoon Suk Rho ^{1,2} and Han Gardeniers ^{2,*}

¹ Department of Instructive Biomaterials Engineering, MERLN Institute for Technology-Inspired Regenerative Medicine, Maastricht University, 6229 ER Maastricht, The Netherlands; h.rho@maastrichtuniversity.nl

² Mesoscale Chemical Systems Group, MESA+ Institute, University of Twente, 7522 NB Enschede, The Netherlands

* Correspondence: j.g.e.gardeniers@utwente.nl; Tel.: +31-(0)53-489-4356

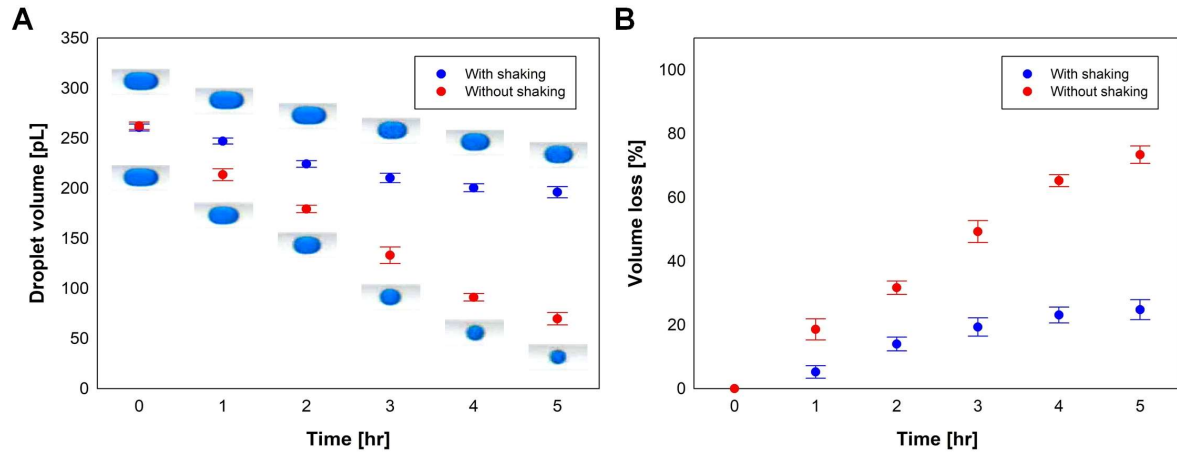


Figure 1. Volume loss of w/o droplets in a non-treated PDMS channel. Three w/o droplets were generated and stored in a storage unit in the microfluidic droplet storage array. Then, the volume change (A) and volume loss rate (B) of the droplets were measured during 5 h incubation at room temperature with shaking (blue) and without shaking (red) (n = 3).