

Supplementary material

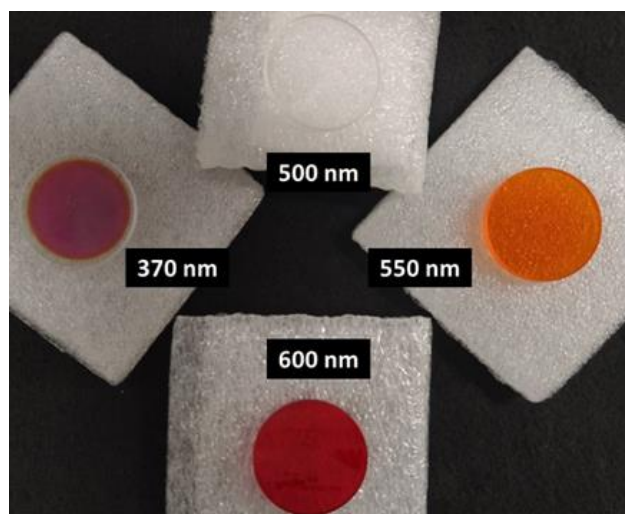
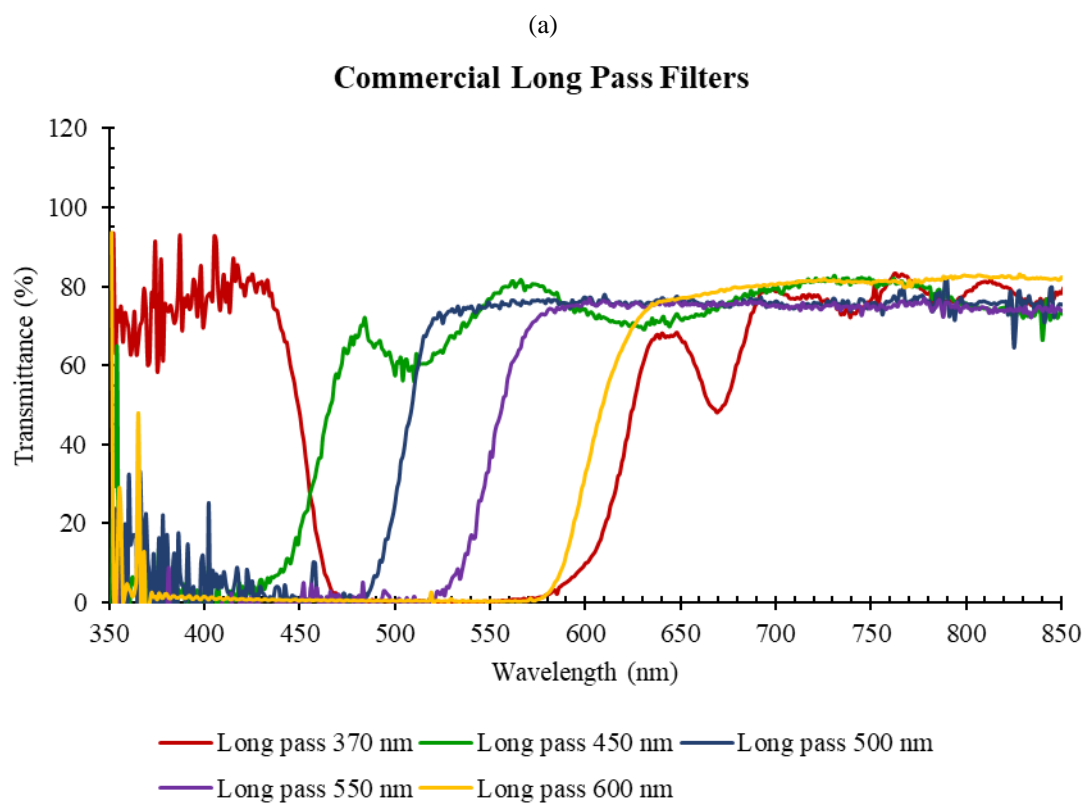


Figure S1: Photographs of examples of the commercial long pass (370 nm, 550 nm and 600 nm) and short pass (500 nm) filters, used in the experimental assays.



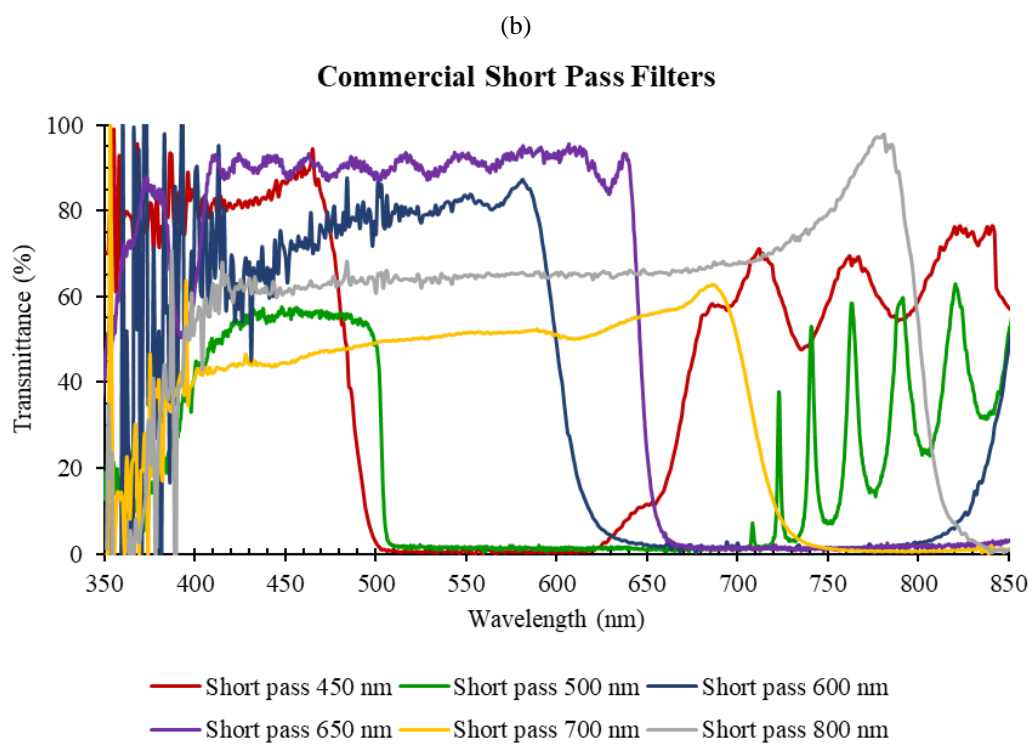


Figure S2: Spectra of the commercial long (a) and short (b) pass optical filters used in the experimental setup and listed in Figure 6 (b).