

Supplementary Information

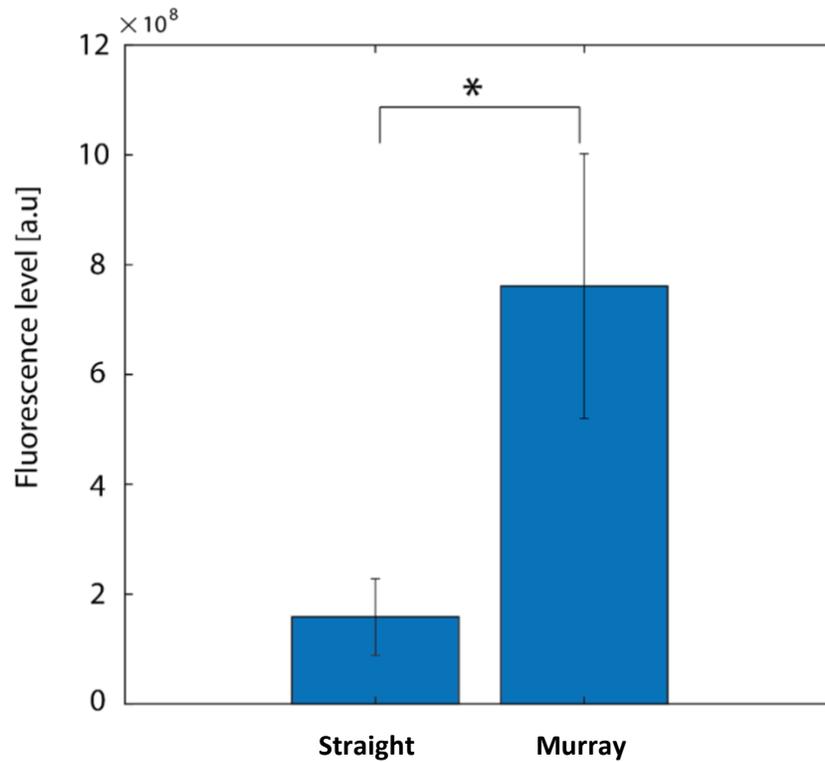


Figure S1. Fluorescence intensity at the final clotting time point (t= 11 min) in collagen coated vascular injury models – straight vs. the Murray model microfluidic device. The bars present the average of the final fluorescence signal in 5 different patients. Significance was determined by unpaired Student's t-test, * $p < 0.05$.