

Supporting information

A Methodologic Approach for the Selection of Bio-Resorbable Polymers in the Development of Medical Devices: The Case of Poly(L-lactide-co- ϵ -caprolactone)

Alberto Cingolani ^{1,2}, Tommaso Casalini ^{1,3}, Stefano Caimi ¹, Antoine Klaue ¹, Mattia Sponchioni ⁴, Filippo Rossi ^{4,*} and Giuseppe Perale ^{2,3,*}

¹ Institute for Chemical and Bioengineering, Department of Chemistry and Applied Bioscience ETH Zurich, Vladimir-Prelog-Weg 1-5/10, 8093 Zürich, Switzerland; alberto.cingolani@chem.ethz.ch (A.C.); tommaso.casalini@chem.ethz.ch (T.C.); stefano.caimi@chem.ethz.ch (S.C.); antoine.klaue@chem.ethz.ch (A.K.)

² Industrie Biomediche Insubri SA (IBI), Via Cantonale 67, 6805 Mezzovico-Vira, Switzerland

³ Biomaterials Laboratory, Institute for Mechanical Engineering and Materials Technology, SUPSI—University of Applied Sciences and Arts of Southern Switzerland, Via Cantonale 2C, Galleria 2, 6928 Manno, Switzerland

⁴ Department of Chemistry, Materials and Chemical Engineering “G. Natta”, Politecnico di Milano, 20100 Milan, Italy; mattia.sponchioni@polimi.it

* Correspondence: filippo.rossi@polimi.it (F.R.); giuseppe.perale@supsi.ch (G.P.); Tel: +39-02-2399-3145 (F.R.); +41-58-666-66-41 (G.P.)

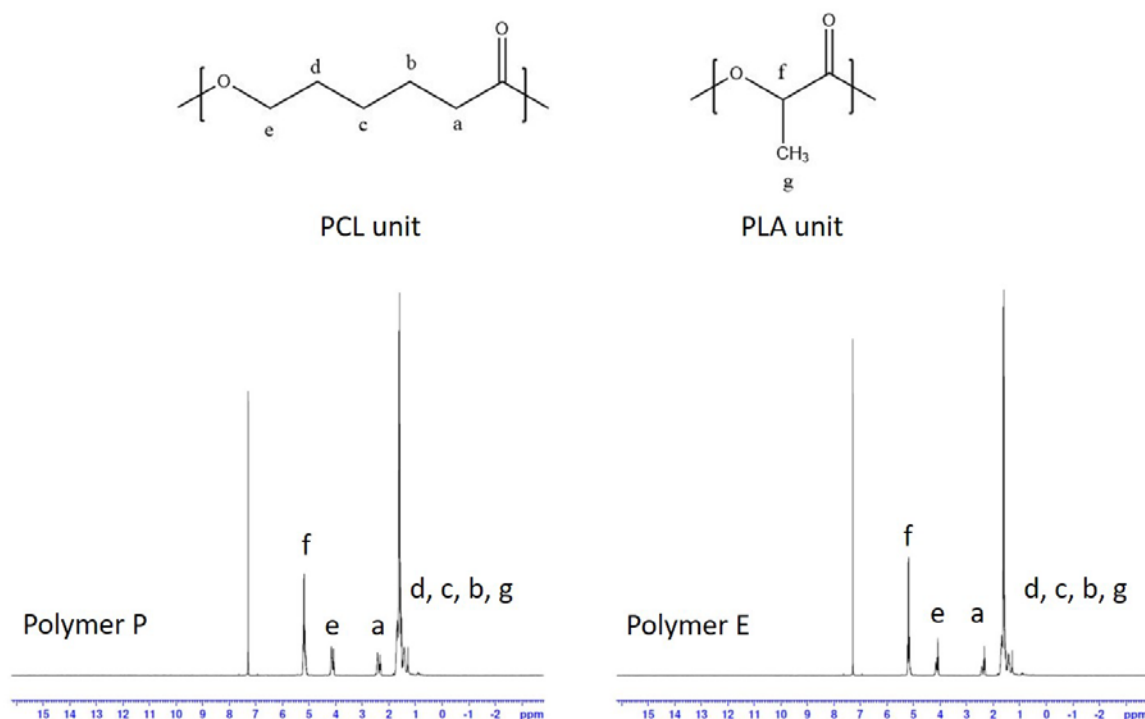


Figure S1. NMR spectra of P and E samples.

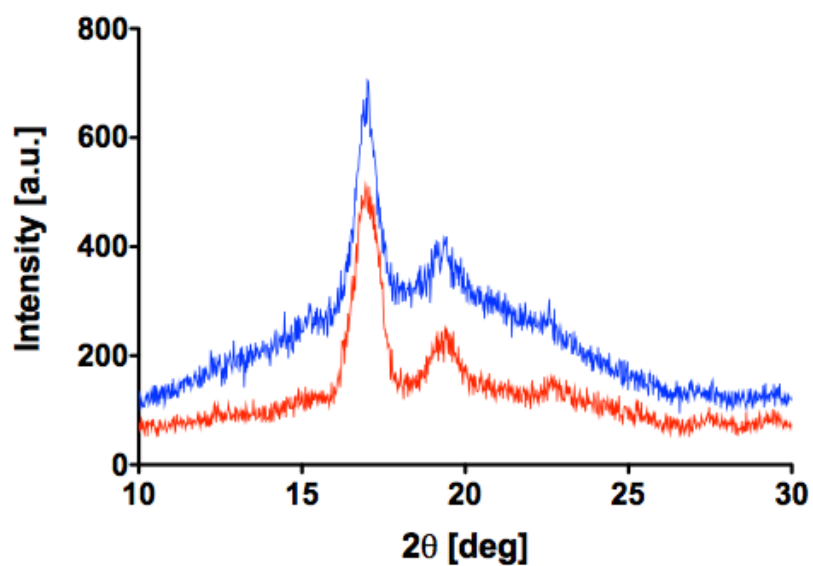


Figure S2. XRD spectra of P (blue line) and E (red line).

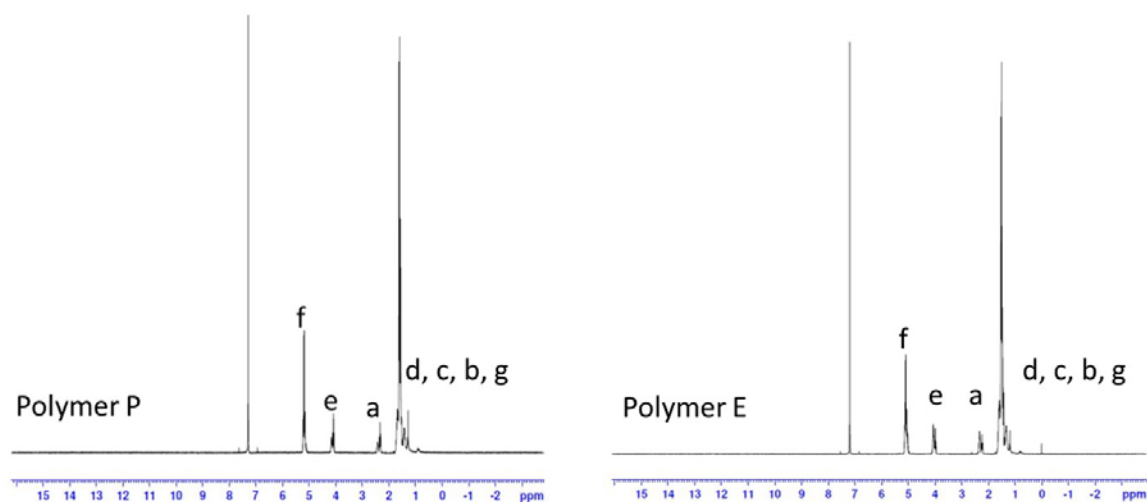


Figure S3. NMR spectra of P and E after EtO.

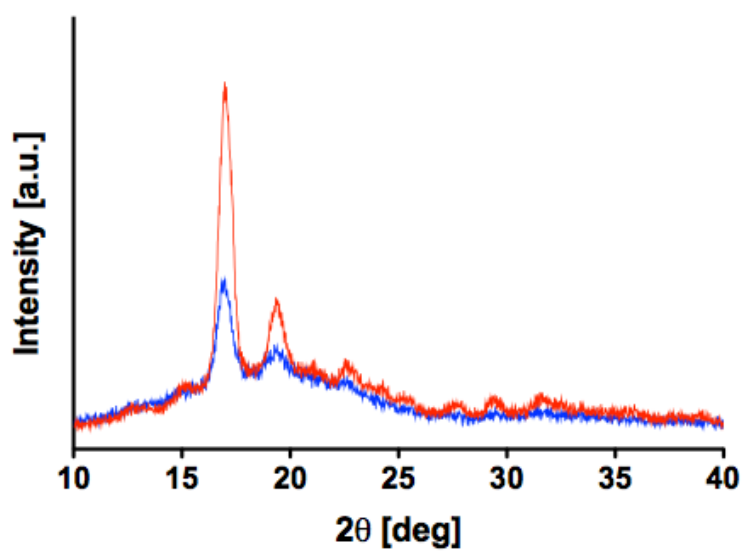


Figure S4. XRD spectra of P (blue line) and E (red line) after EtO.

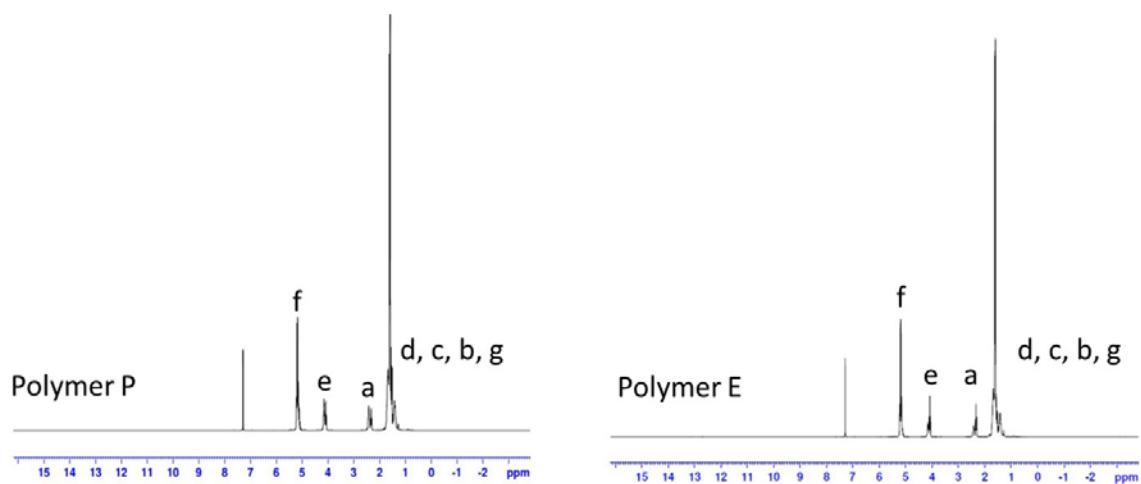


Figure S5. NMR spectra of P and E after electron beam irradiation.

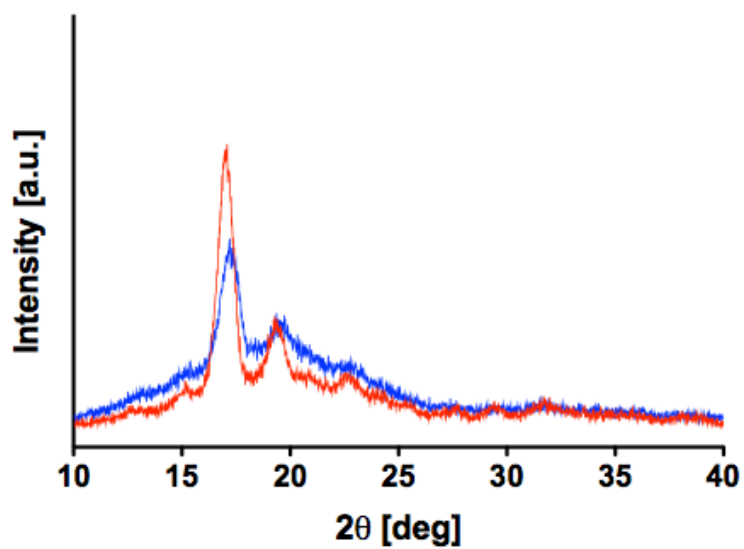


Figure S6. XRD spectra of P and E after electron beam irradiation.



© 2018 by the authors. Submitted for possible open access publication under the terms and conditions of the Creative Commons Attribution (CC BY) license (<http://creativecommons.org/licenses/by/4.0/>).