



Finger-Actuated Microneedle Array for Sampling Body Fluids

Misagh Rezapour Sarabi, Abdollah Ahmadpour, Ali K. Yetisen and Savas Tasoglu

Supplementary Information

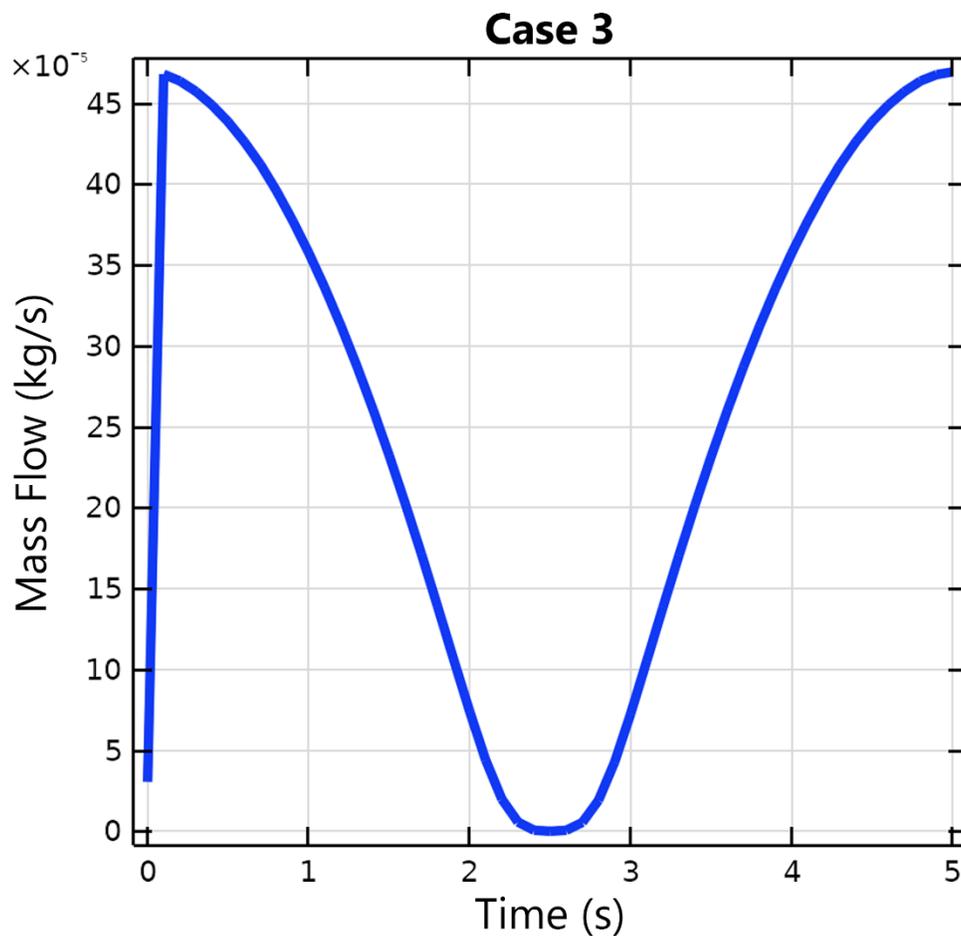

Supplementary Figure S1 - Mass flow curve result at the reservoir for Case 3 in Table 3. The curve shows the mass flow rate in $\text{kg}\cdot\text{s}^{-1}$ for time in seconds. Time duration is 5 s.

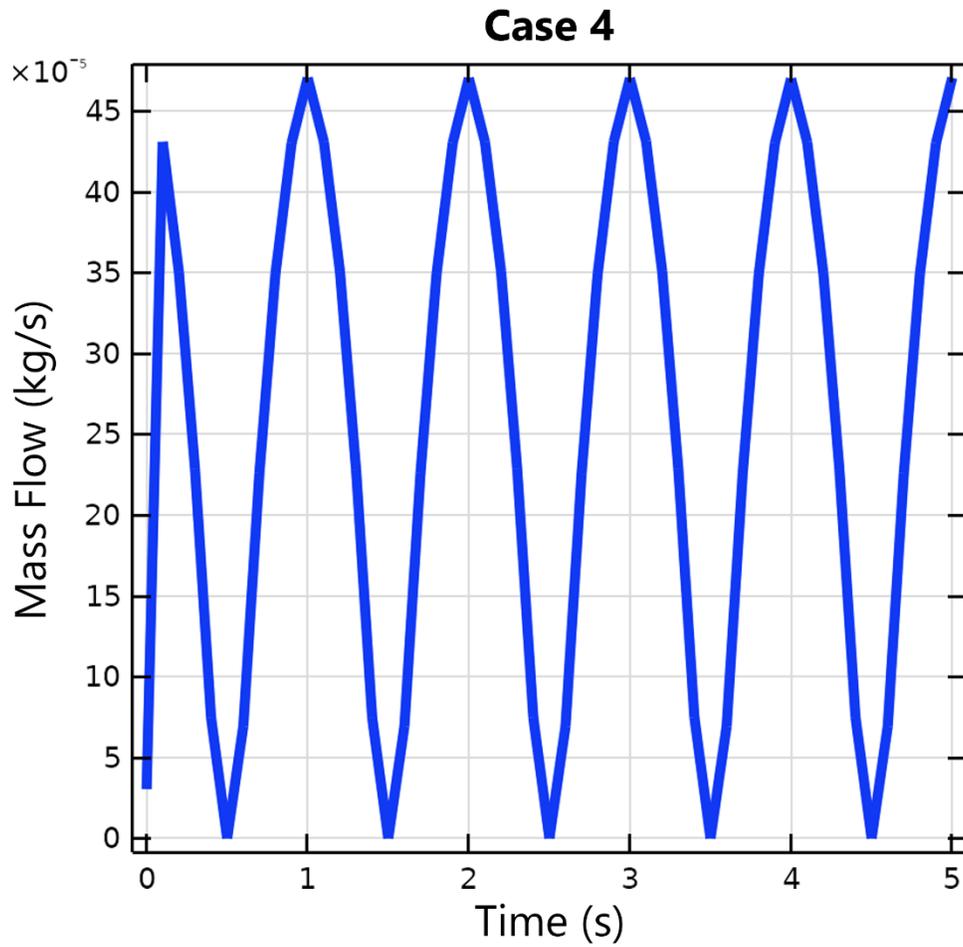

Supplementary Figure S2 - Mass flow curve result at the reservoir for Case 4 in Table 3. The curve shows the mass flow rate in kg.s^{-1} for time in seconds. Time duration is 5 s.