

Optimizing CNT Loading in Antimicrobial Composites for Urinary Tract Application

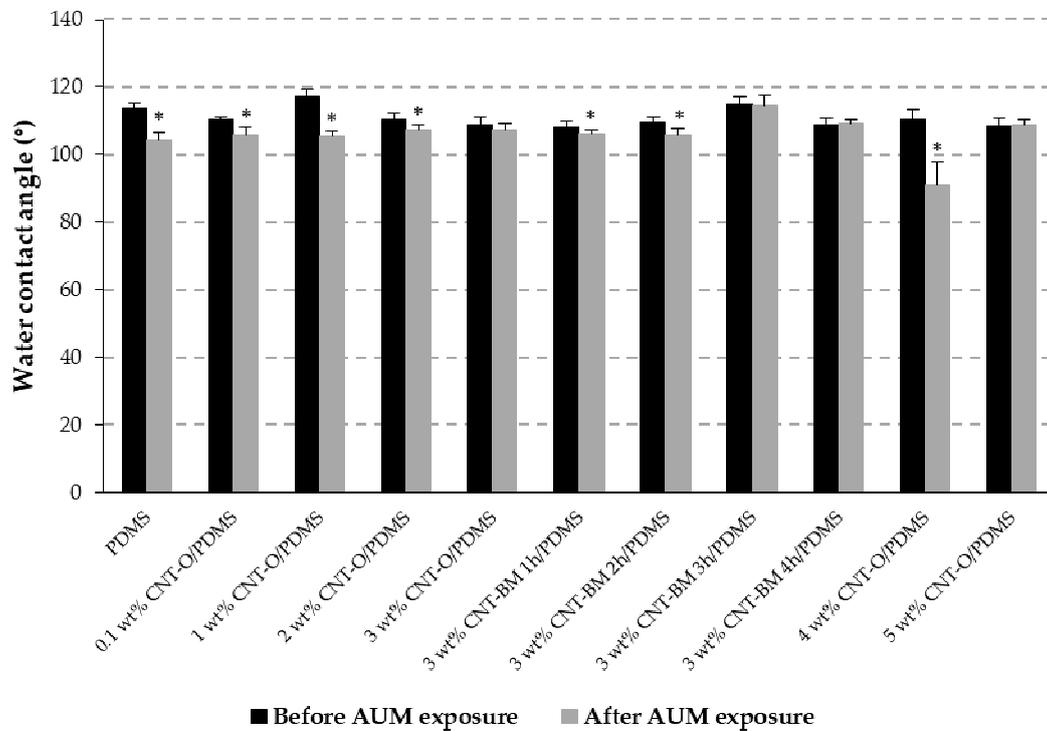


Figure 1. Water contact angles before (■) and after 24-h exposure (■) to artificial urine medium (AUM). Values are means \pm standard deviations (SDs) of three independent experiments. Significant differences before and after medium exposure were considered for p -values < 0.05 (*).