



Supplementary Materials

Reduced Graphene Oxide and Gold Nanoparticles-Modified Electrochemical Aptasensor for Highly Sensitive Detection of Doxorubicin

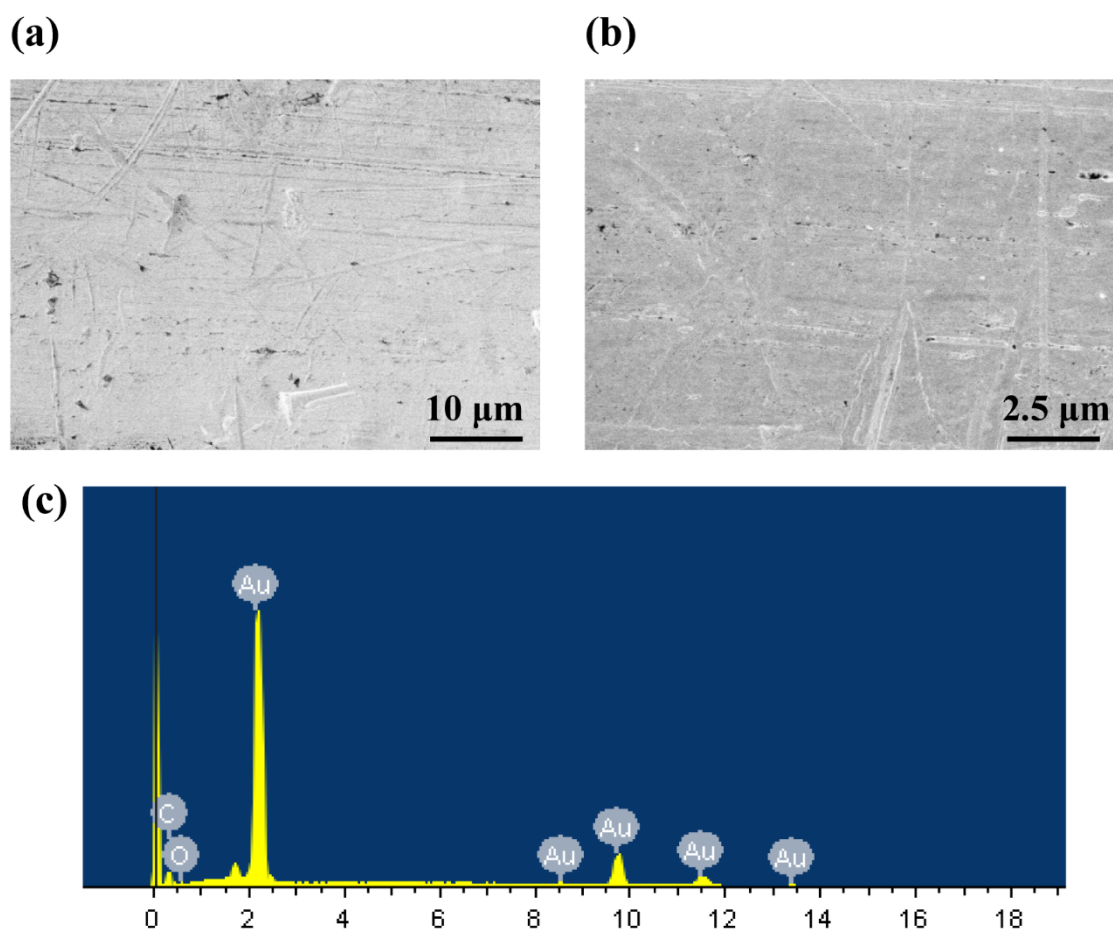


Figure S1. (a,b) Scanning electron microscope (SEM) images of bare electrode at different scales; (c) The energy dispersive X-Ray spectrometer (EDS) of the rGO/AuNPs modified electrode.