

Article

Evaluation of Antimicrobial Performance of Calcium Dihydroxide (Ca(OH)₂) Coating on Ti for Potential Metallic Orthopedic Implant Applications

Harald Holeczek ^{1,2}, Michael de Wild ³, Jasmine Ruegg ³, Philipp Gruner ¹, Walter Moser ⁴ and Olivier Braissant ^{5,*}

¹ Medicoat AG, Almuesenacherstrasse 2, 5506 Mägenwil, Switzerland; h.holeczek@medicoat.ch (H.H.);

² Fraunhofer-Institut für Produktionstechnik und Automatisierung IPA, Nobelstr. 12, 70569 Stuttgart, Germany

³ Fachhochschule Nordwestschweiz FHNW, Campus Muttens, Hofackerstrasse 30, 4132 Muttens, Switzerland; michael.dewild@fhnw.ch (M.d.W.)

⁴ Atesos Medical AG, Schachenallee 29, 5000 Aarau, Switzerland

⁵ Department of Biomedical Engineering, University of Basel, Hegenheimermattweg 167B/C, CH-4123 Allschwil, Switzerland

* Correspondence: olivier.braissant@unibas.ch (O.B)

Academic Editor: Marc Maresca

Received: 18 September 2024


Revised: 7 January 2025

Accepted: 10 January 2025

Published: 14 January 2025

Citation: Holeczek, H.; de Wild, M.; Ruegg, J.; Gruner, P.; Moser, W.; Braissant, O. Evaluation of Antimicrobial Performance of Calcium Dihydroxide (Ca(OH)₂) Coating on Ti for Potential Metallic Orthopedic Implant Applications. *Antibiotics* **2025**, *14*, x. <https://doi.org/10.3390/xxxxx>

Copyright: © 2025 by the authors. Submitted for possible open access publication under the terms and conditions of the Creative Commons Attribution (CC BY) license (<https://creativecommons.org/licenses/by/4.0/>).

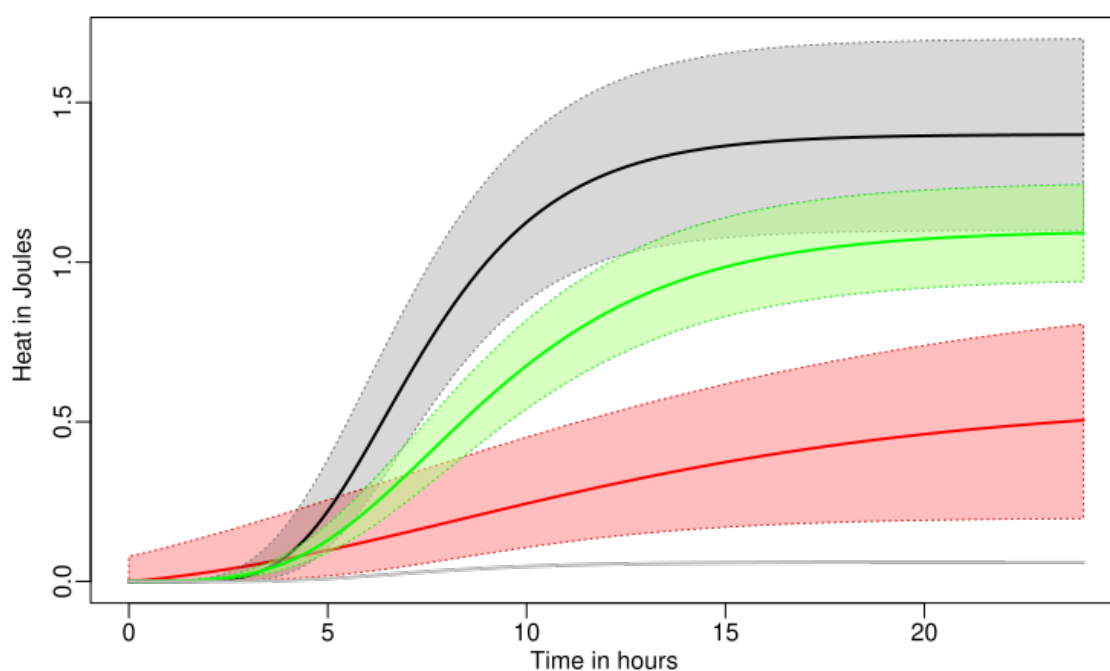

Supplementary Figure S1. Growth of *S. epidermidis* (A) (10⁵ inoculum) at the surface of uncoated (green), HA coated (black) and Ca(OH)₂ coated (red) screws. The growth curves were redrawn using the values from the growth parameters in table 3. Plain lines indicate the average growth pattern, clear areas limited by dashed lines indicate the standard deviation.