

Article

# Novel Synthesis of Core-Shell Biomaterials from Polymeric Filaments with a Bioceramic Coating for Biomedical Applications

Catalina-Andreea Dascalu <sup>1</sup>, Florin Miculescu <sup>1,\*</sup>, Aura-Catalina Mocanu <sup>1</sup>, Andreea Elena Constantinescu <sup>1</sup>, Tudor Mihai Butte <sup>1</sup>, Andreea Madalina Pandeale <sup>2,3</sup>, Robert-Catalin Ciocoiu <sup>1</sup>, Stefan Ioan Voicu <sup>2</sup>, Lucian Toma Ciocan <sup>4</sup>

<sup>1</sup> Department of Metallic Materials Science, Physical Metallurgy, University Politehnica of Bucharest, 060042 Bucharest, Romania; catalina.dascalu@hotmail.com (C.A.D.); f\_miculescu@yahoo.com (F.M.);

mcn\_aura@hotmail.com (A.C.M.); andreeaelena01c@gmail.com (A.E.C.); butte.tudor@yahoo.com (T.M.B.)


<sup>2</sup> Department of Analytical Chemistry and Environmental Engineering, University Politehnica of Bucharest, 011061 Bucharest, Romania; pandele.m.a@gmail.com (A.M.P.); svoicu@gmail.com (S.I.V.)

<sup>3</sup> Advanced Polymer Materials Group, University Politehnica of Bucharest, 011061 Bucharest, Romania

<sup>4</sup> Prosthetics Technology and Dental Materials Department, University of Medicine and Pharmacy, 020022 Bucharest, Romania; tcioacan@yahoo.com

\* Correspondence: f\_miculescu@yahoo.com; Tel.: +40-21-3169563

Received: 12 February 2020; Accepted: 15 March 2020; Published: date

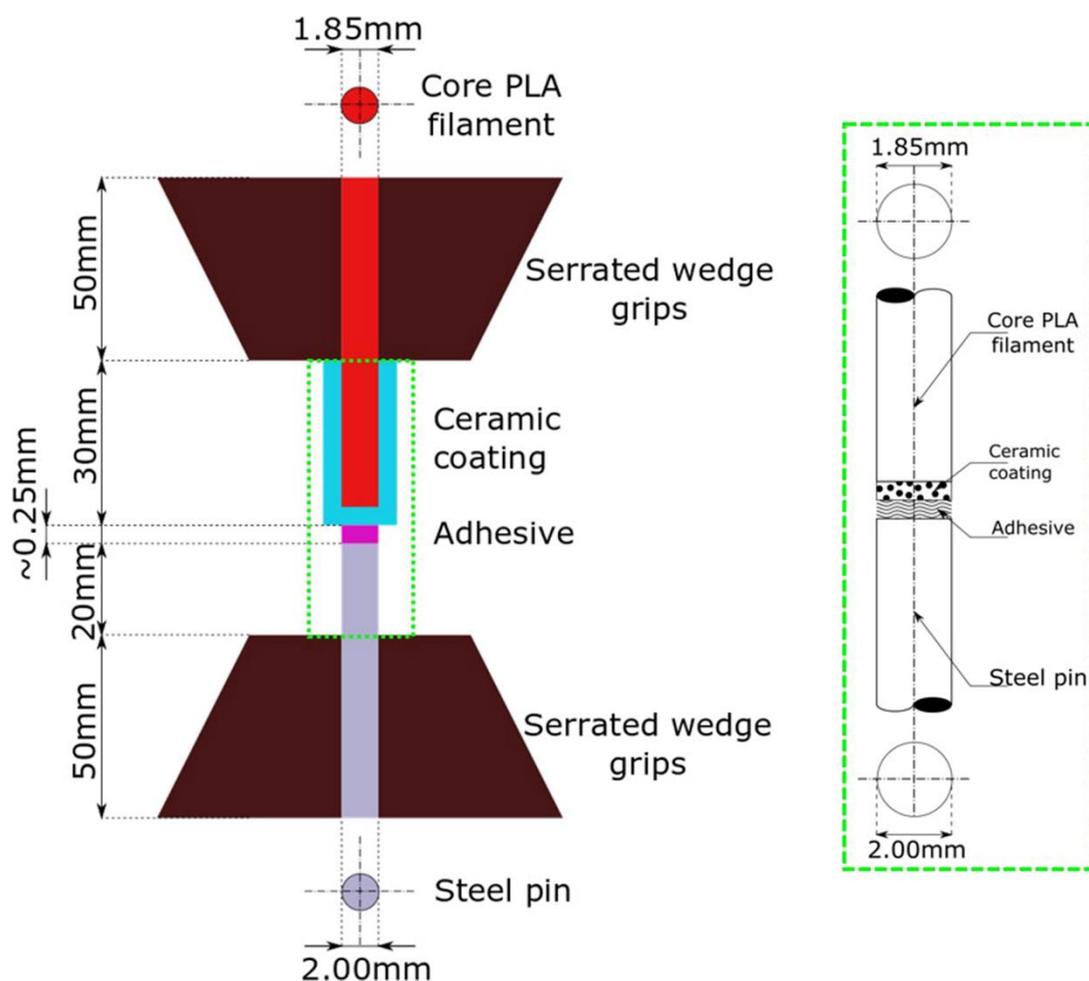

**Figure S1.** Schematic representation for the adapted preparation method of the pull-out test samples.

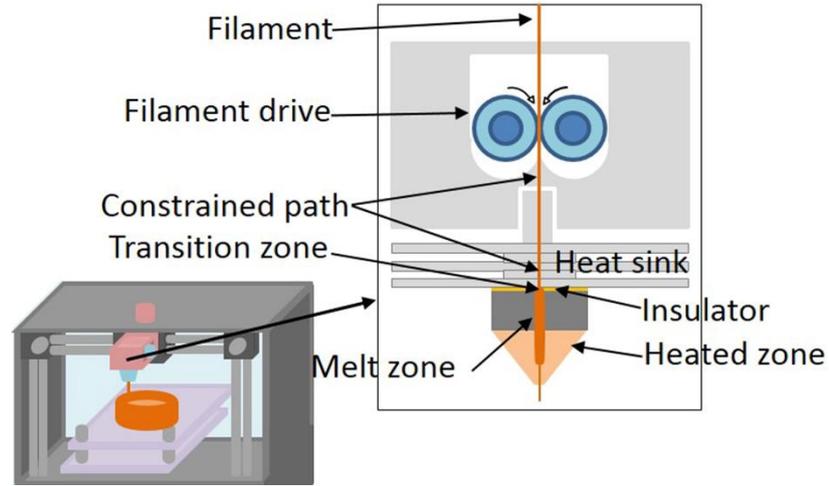


Figure S2. Schematic representation of the filament travel route inside of a 3D printer.

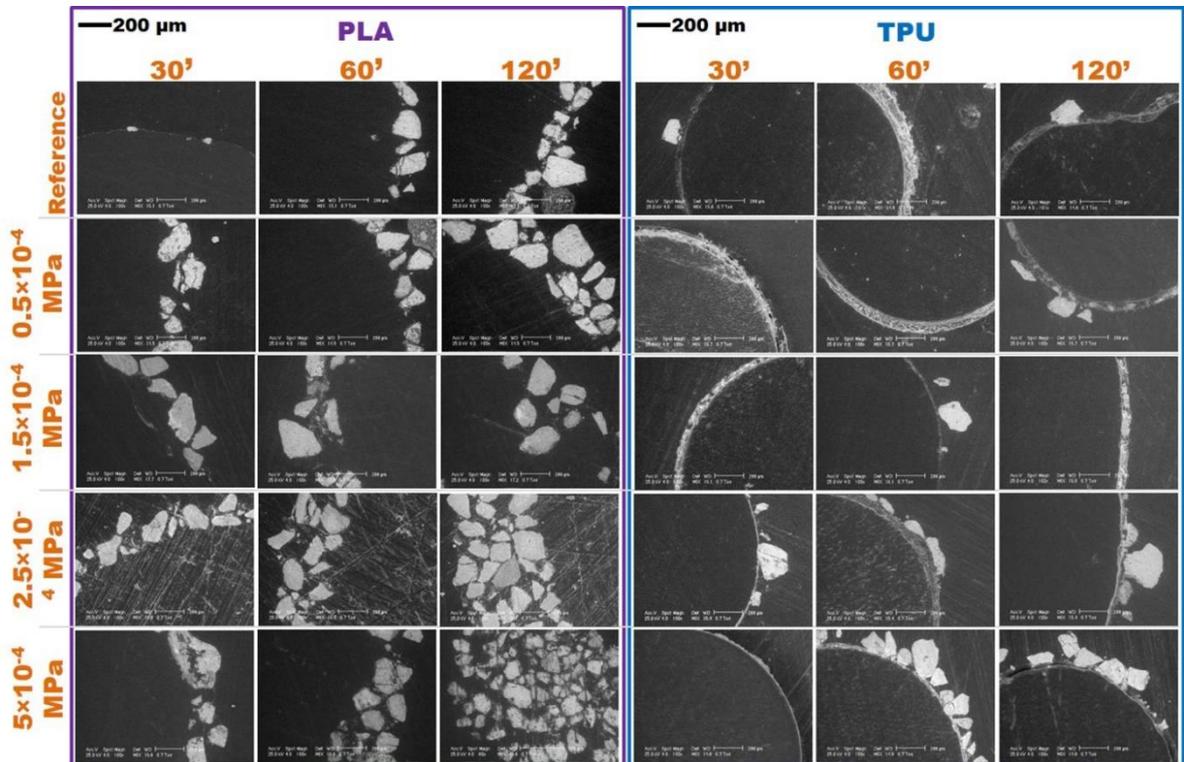


Figure S3. Form factor variation at 195 °C temperature at higher magnifications.

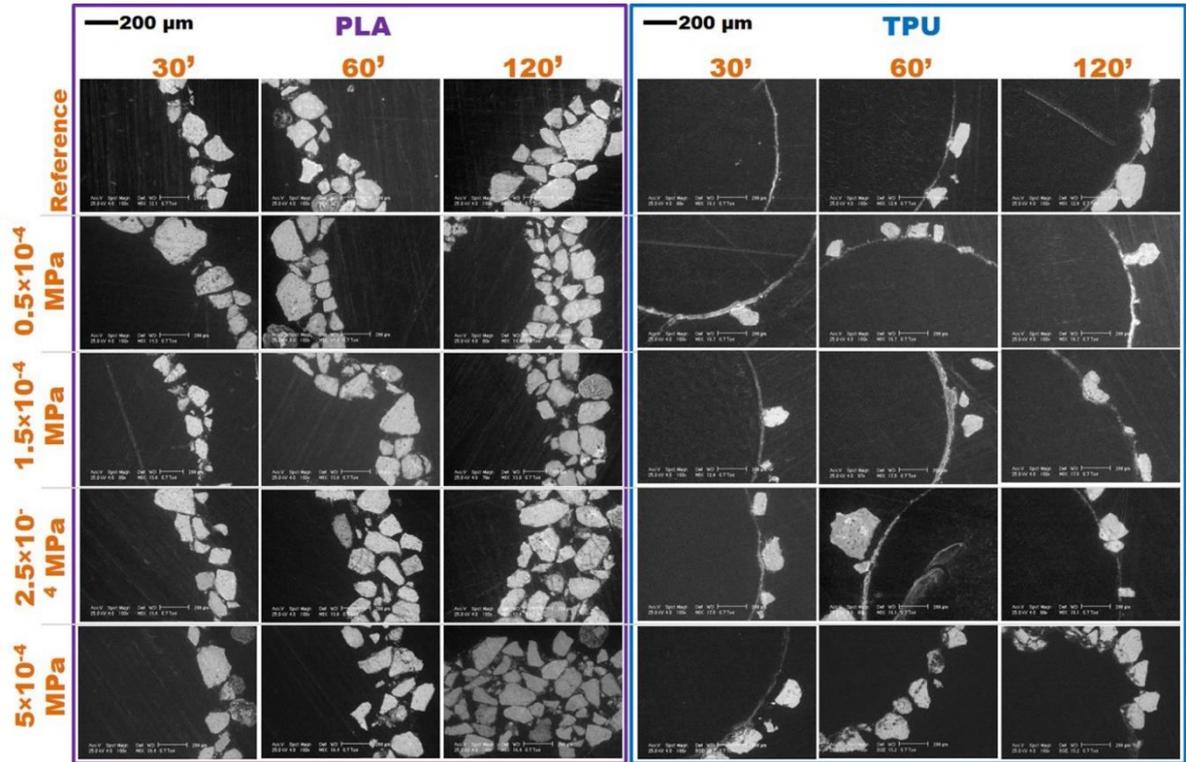


Figure S4. Form factor variation at 205 °C temperature at higher magnifications.

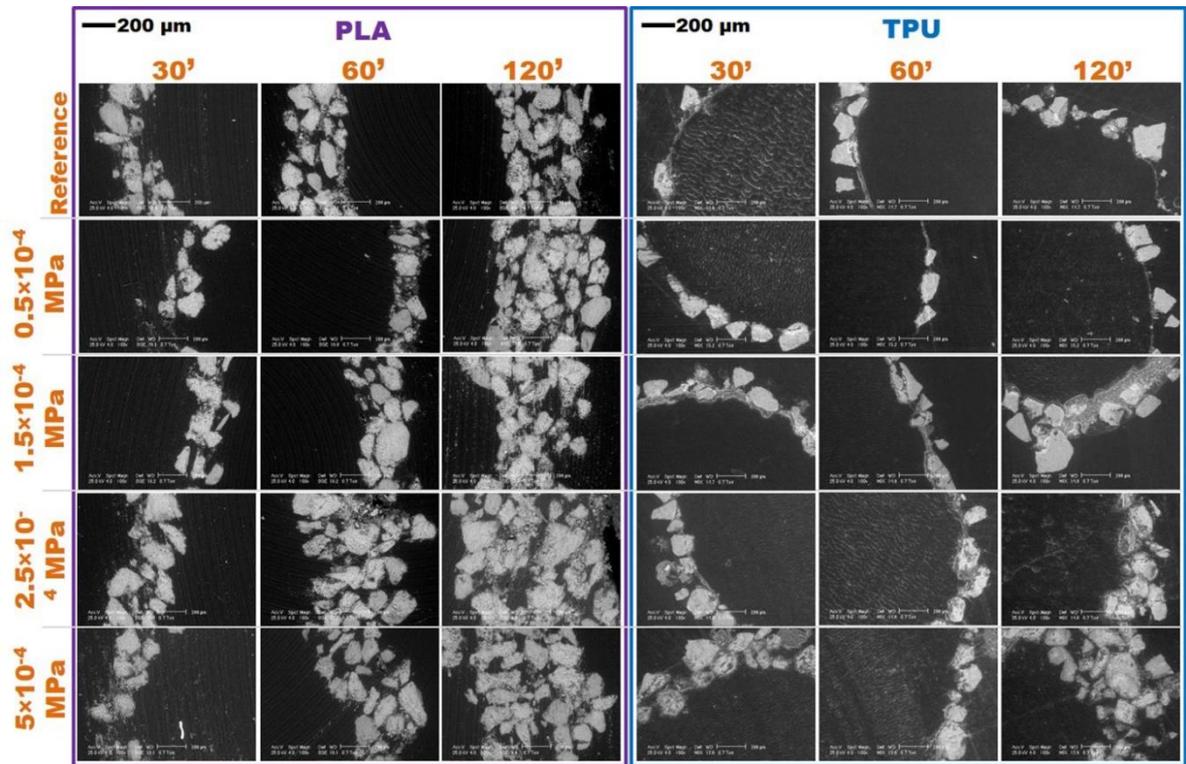


Figure S5. Form factor variation at 215 °C temperature at higher magnifications.



