

## Supporting information

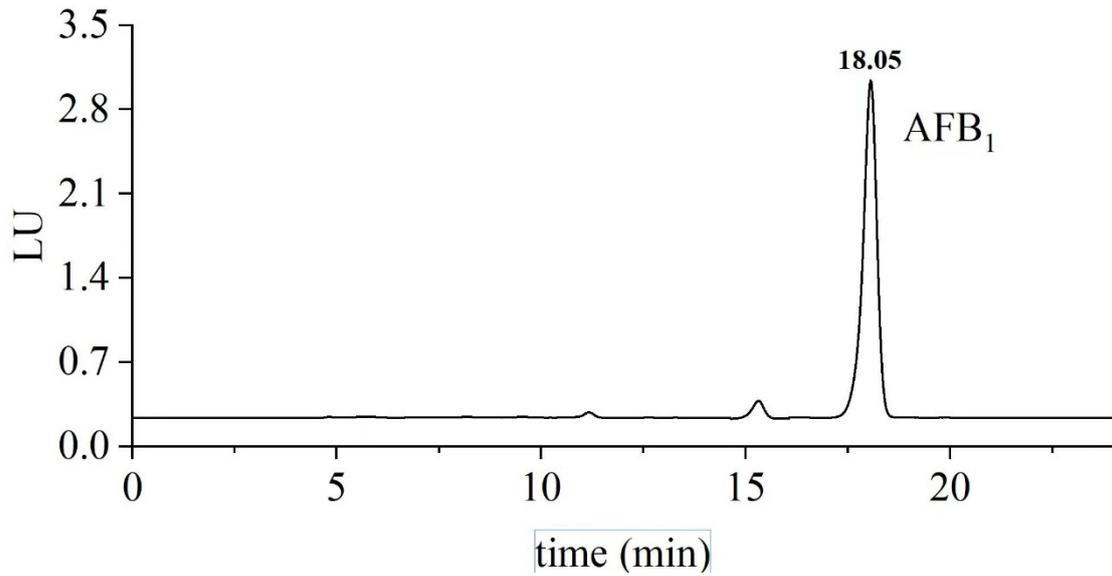


Figure S1. The quantity of AFB<sub>1</sub> was measured using an HPLC system

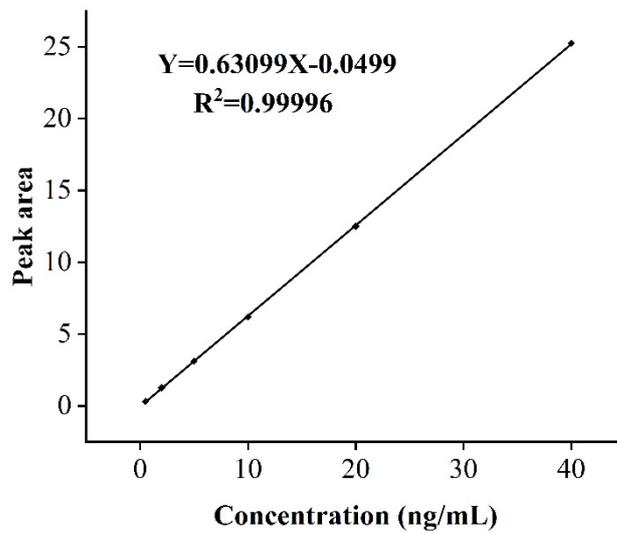


Figure S2. The Standard curve of AFB<sub>1</sub> measured by HPLC