

Figure S1: Auto-aggregation test. The OD at 610 nm of a suspension of 10^7 CFU/mL of each yeast strain was measured every 10 min for 60 min without disturbances.

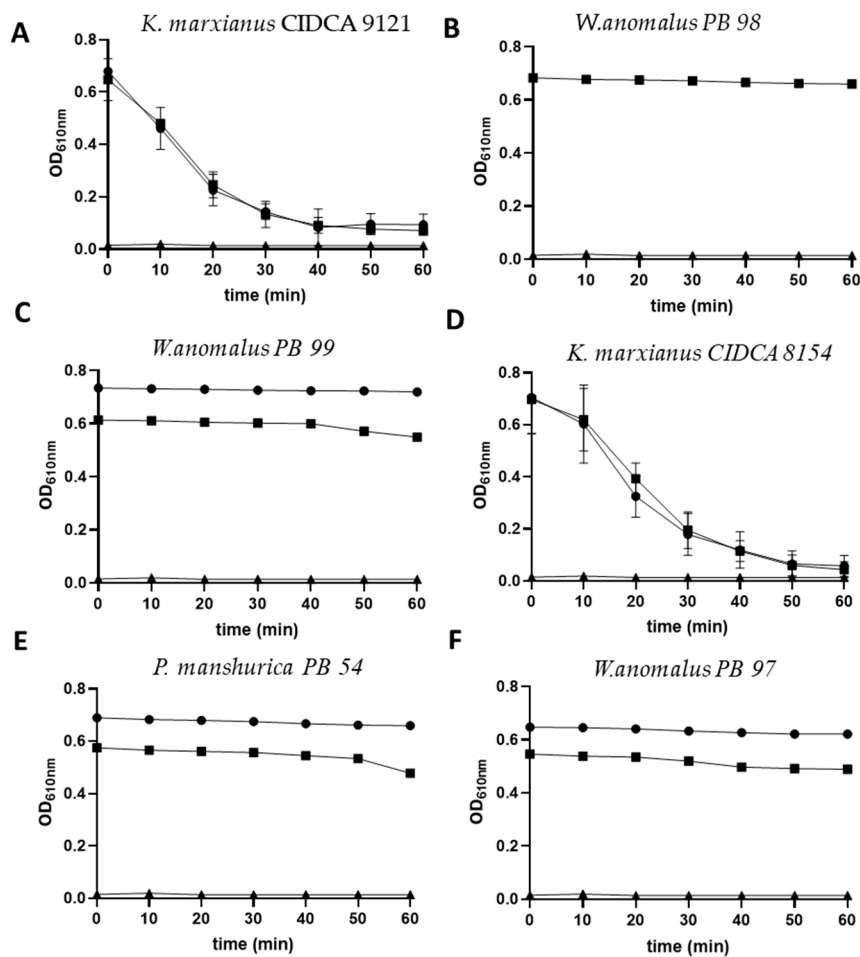


Figure S2: Co-aggregation test. The OD at 610 nm of a mixed suspension of 10^7 CFU/mL of each yeast strain and 10^7 CFU/mL of *S. Enteritidis* was measured every 10 min for 60 min without disturbances (black square). Auto-aggregation test is also shown for each yeast (black circle) and for *S. Enteritidis* (black triangle)